


AN 435

Accurate Dosimetry for High Dose Plasma Implanted Boron using EAGLABSSM PCOR-SIMSSM

May 9, 2007 (Version 2.0)

Discussion

High dose plasma implantation of boron into silicon results in boron surface concentrations well into the % range and in many cases, well into the 10s of % range. Traditionally, the linearity of SIMS quantification breaks down once percent levels of a dopant or impurity are reached and quantification accuracy is reduced. Quantification is further complicated by the presence of surface oxide and again by changing sputter rates as a function of boron and oxygen concentration.

At EAG, we have taken all of these effects into consideration and have developed a new analysis protocol (**EAGLABSSM PCOR-SIMS^{*}** for ULE B). The result is an accurate boron concentration vs. depth curve in the critical high concentration region that provides best-ever SIMS dosimetry for high dose, high concentration implants.

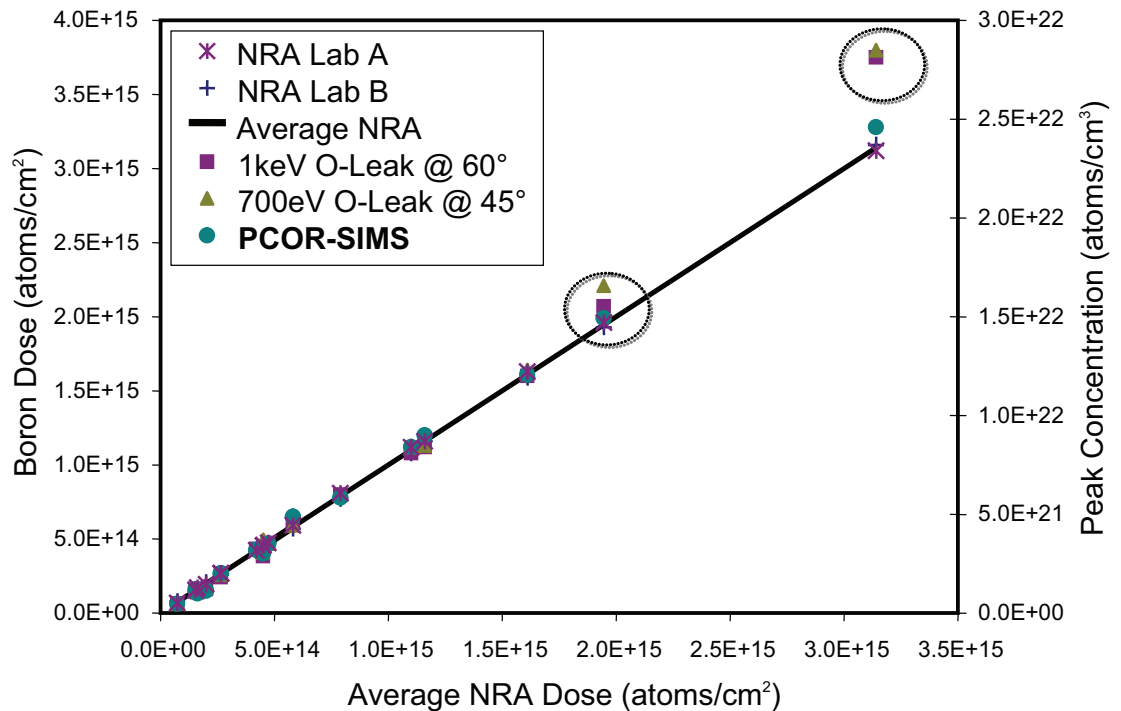


Figure 1. SIMS dosimetry is compared with NRA from 2 independent laboratories. SIMS and NRA dosimetry using all analysis protocols are good up to about $1.5E+15$ at/cm^2 dose. Above this concentration, only **PCOR-SIMS** for ULE B accurately takes sensitivity factor and sputter rate effects into account and reports accurate dosimetry.

* The new PCOR-SIMSSM for ULE B protocol is the result of extensive development efforts by EAG. The "PCOR-SIMSSM" name describes, in part, EAG's proprietary methodology that includes point-to-point correction resulting in the most accurate SIMS profiling yet for ultra shallow implants.

United States Locations

Tempe, Arizona
+1 480 239 0602 info.az@eaglabs.com
+1 602 470 2655 fax

Sunnyvale, California
810 Kifer Road
+1 408 530 3500 info.ca@eaglabs.com
+1 408 530 3501 fax

1135 E Arques Avenue
+1 408 738 3033
+1 408 738 3035 fax

785 Lucerne Drive
+1 408 737 3892
+1 408 737 3916 fax

Peabody, Massachusetts
+1 978 278 9500 info.ma@eaglabs.com
+1 978 278 9501 fax

Chanhassen, Minnesota
+1 952 828 6411 info.mn@eaglabs.com
+1 952 828 6449 fax

East Windsor, New Jersey
+1 609 371 4800 info.nj@eaglabs.com
+1 609 371 5666 fax

Syracuse, New York
+1 315 431 9900 info.ny@eaglabs.com
+1 315 431 9800 fax

Raleigh, North Carolina
+1 919 829 7041 info.nc@eaglabs.com
+1 919 829 5518 fax

Round Rock, Texas
+1 512 671 9500 info.tx@eaglabs.com
+1 512 671 9501 fax

International Locations

Shanghai, China
+ 86 21 6879 6088 info.cn@eaglabs.com
+ 86 21 6879 9086 fax

Tournefeuille, France
+ 33 5 61 73 15 29 info.fr@eaglabs.com
+ 33 5 61 73 15 67 fax

Frankfurt, Germany
+ 49 (0) 693053213 info.de@eaglabs.com
+ 49 (0) 69307941 fax

Tokyo, Japan
+ 81 3 5396 0531 info.jp@eaglabs.com
+ 81 3 5396 1930 fax

HsinChu, Taiwan
+ 886 3 5632303 info.tw@eaglabs.com
+ 886 3 5632306 fax

Uxbridge, United Kingdom
+ 44 (0) 1895 811194 info.uk@eaglabs.com
+ 44 (0) 1895 810350 fax